



Cryogenic Operation
in Building 902A
January – January, 2005

K. C. Wu
2/7/2005


No. of Tests (Vertical plus Horizontal) per Month in 2005

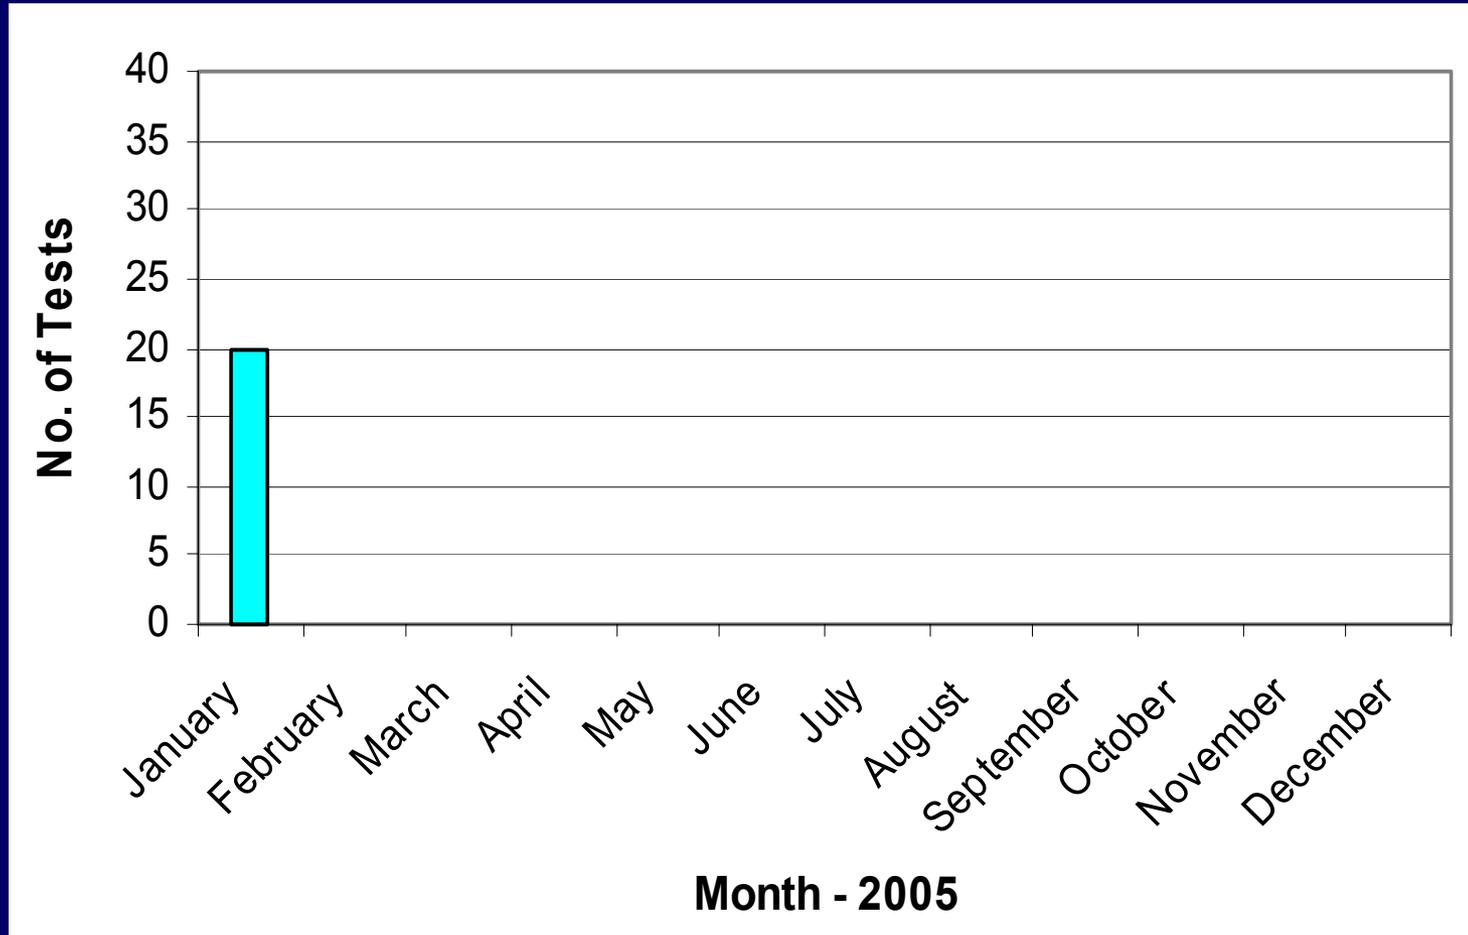


Helium Liquefaction Rate - Gallon per Hour January - January, 2005

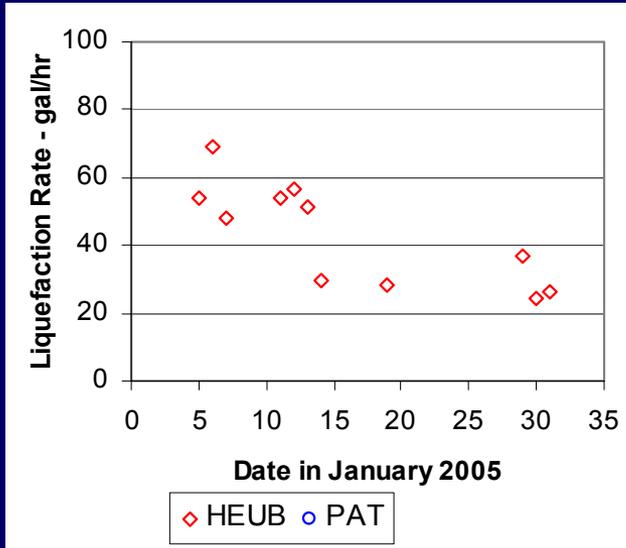


Overnight LN₂ Usage - Liter per Hour January - January, 2005

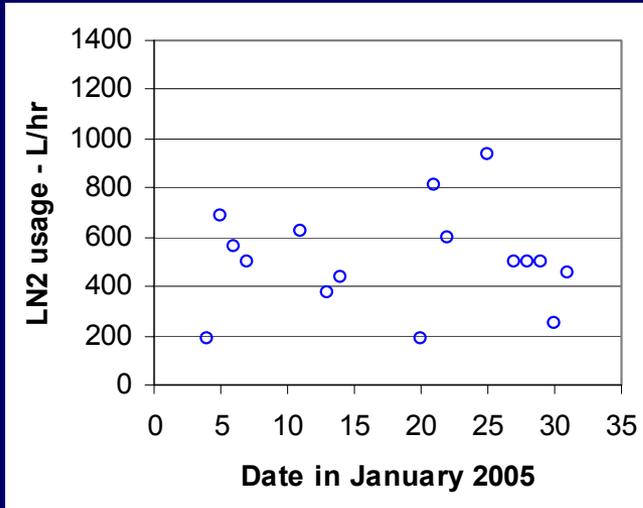


Monthly Charge of Helium Gas in 2005

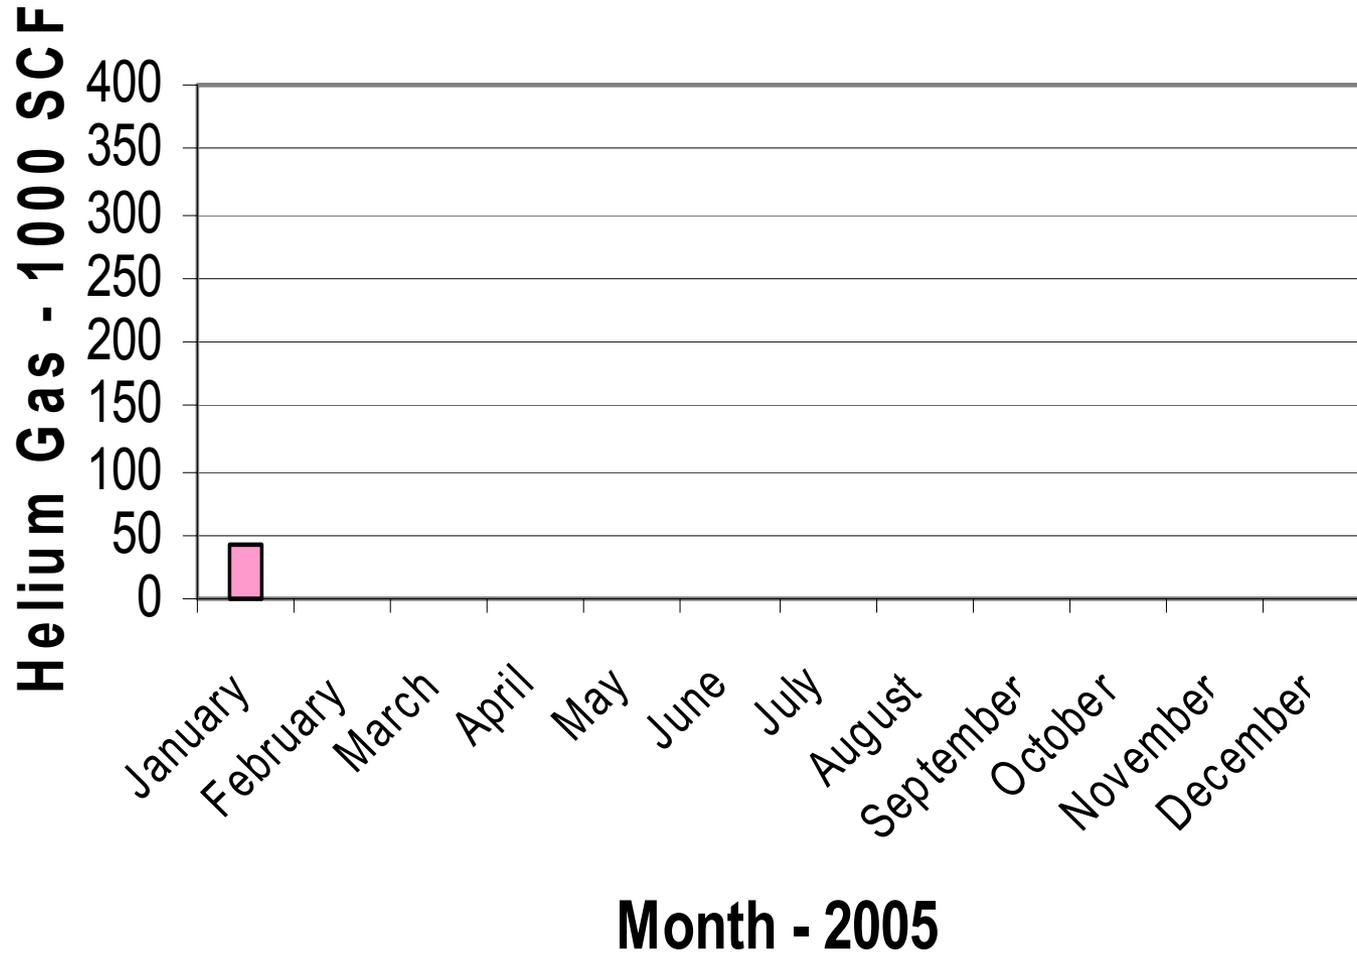


Monthly Liquid Helium Provided to On-site User from B902 in 2005

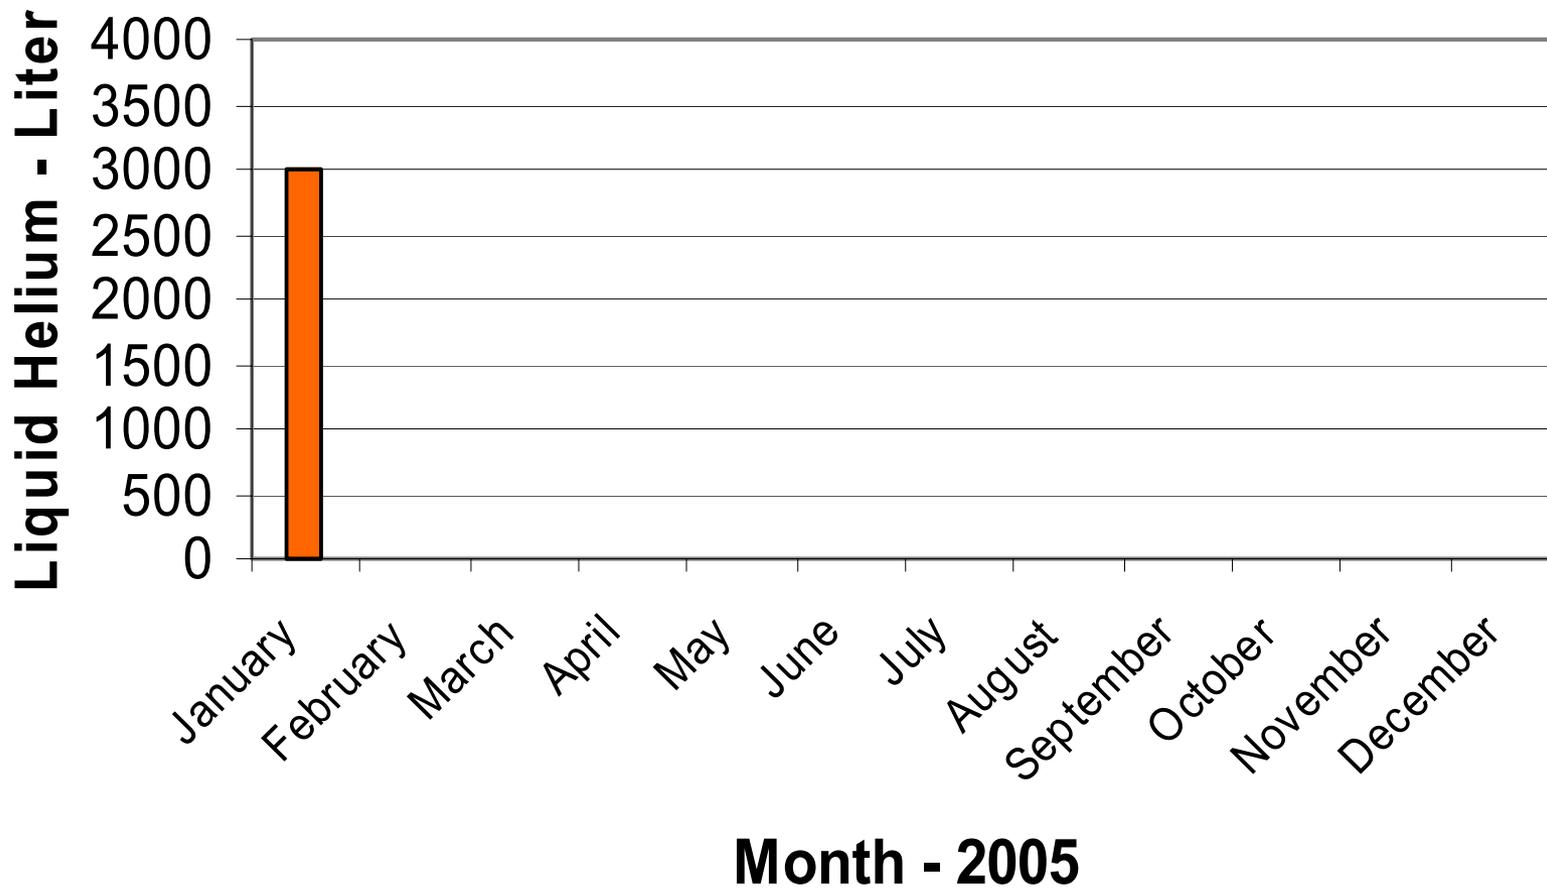


Monthly Charge of Liquid Nitrogen in 2005

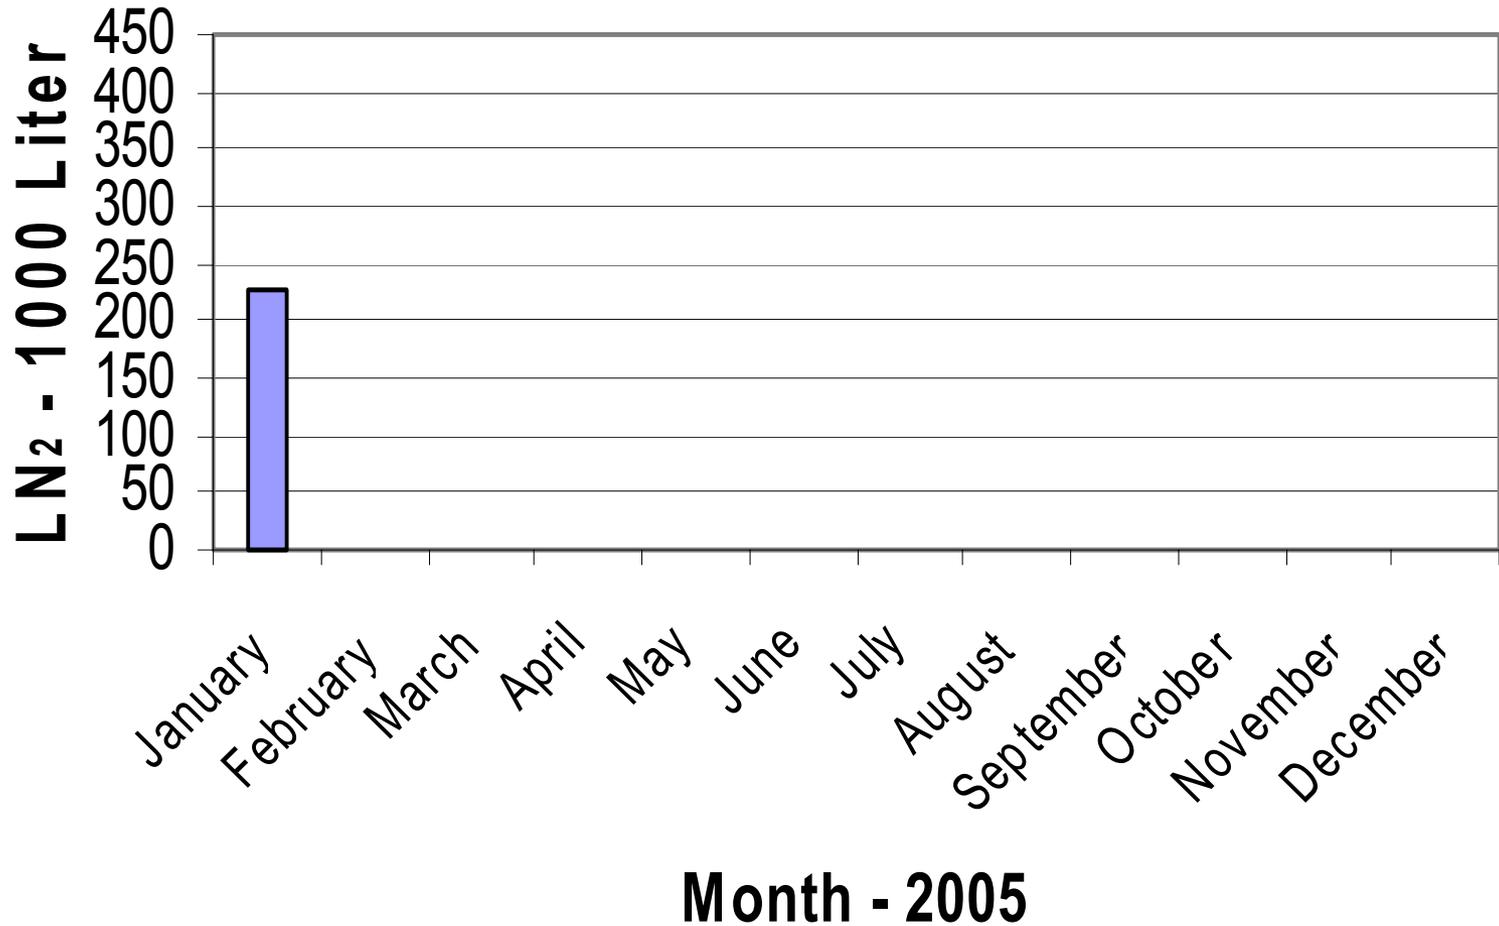

Total Liquid Helium Provided to On-site User from B902 in 2005

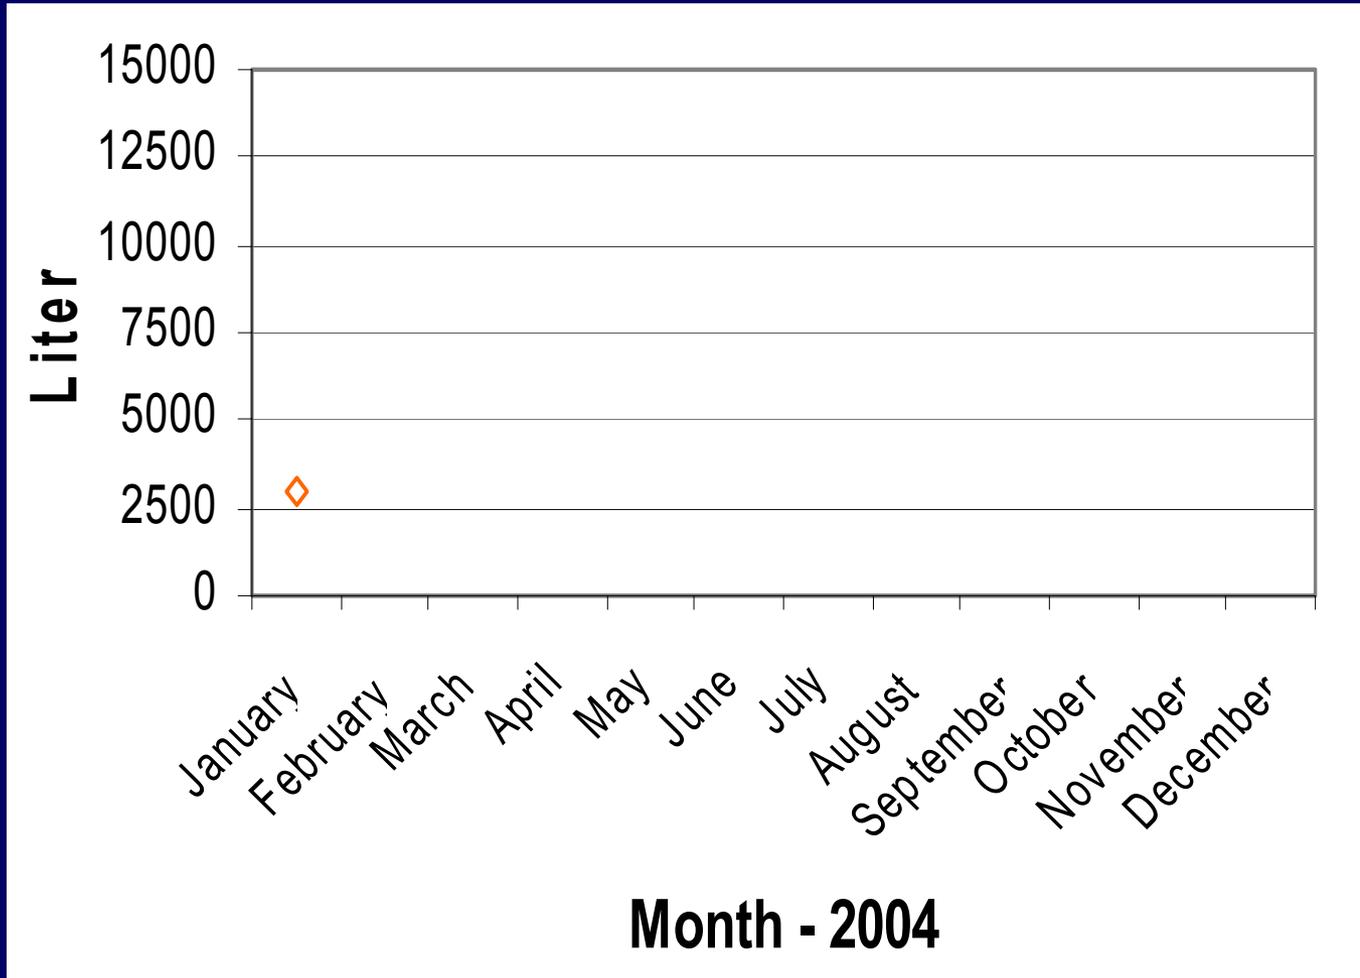

Cumulative Cost of Cryogen in B902 - 2005

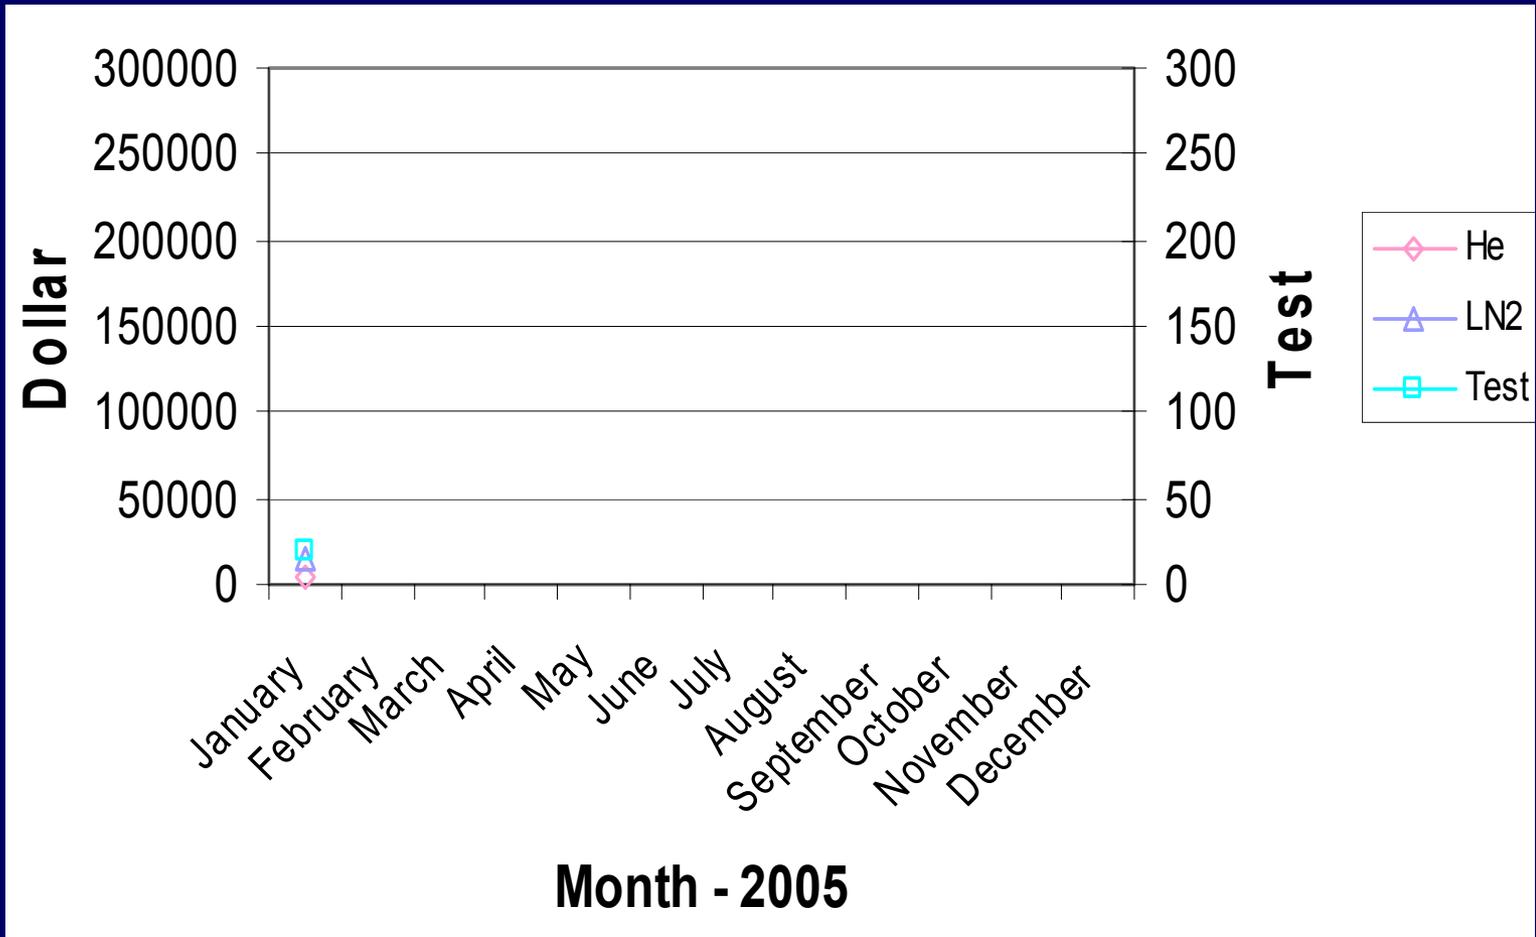

Daily Record of Helium Inventory January - January, 2005

