



Collection of groundwater samples using one of the Lab's drilling rigs.

Chapter 9

Quality Assurance



Quality Assurance is an integral part of every activity at Brookhaven National Laboratory (BNL).

A comprehensive Quality Assurance/Quality Control (QA/QC) Program is in place to ensure that all environmental monitoring samples are representative, and that data are reliable and defensible. Most analyses are performed by contract laboratories that are state certified and routinely participate in independent performance testing. QC at the analytical laboratories is maintained through daily instrument calibration, efficiency, background checks, and testing for precision and accuracy. Data are verified and validated, as required, by project-specific quality objectives before being used to support decision making. The multilayered components of QA monitored at BNL ensure that all analytical data reported for the 2024 Site Environmental Report (SER) are reliable and of acceptable quality.

9.1

Quality Program Elements

As required by the Department of Energy (DOE), BNL has established a QA/QC Program to ensure that the accuracy, precision, and reliability of environmental monitoring data are consistent with the requirements of Title 10 of the Code of Federal Regulations, Part 830, Subpart A, Quality Assurance Requirements, and DOE Order 414.1D, Quality Assurance. The responsibility for quality at BNL starts with the Laboratory Director, who approves the policies and standards of performance governing work that extends throughout the entire organization. The purpose of the BNL QA Program is to implement QA methodology throughout the various Laboratory management systems and associated processes to do the following:


- Plan and perform operations in a reliable and effective manner to minimize any impact on the environment, safety, security, and health of the staff and public.
- Standardize processes and support continual improvement.
- Enable the delivery of products and services that meet customers' requirements and expectations.
- Support an environment that facilitates scientific and operational excellence.

For environmental monitoring, QA is deployed as an integrated system of management activities. These activities involve planning, implementation, control, reporting, assessment, and continual improvement. QC activities measure each process or service against the QA standards. QA/QC practices and procedures are documented in manuals, plans, and a comprehensive set of Standard Operating Procedures (SOPs) for environmental monitoring (EM-SOPs). Staff members who must follow these procedures are required to document that they have reviewed and understand them.

The goal of the environmental monitoring and analysis QA/QC program is to ensure that results are representative and defensible, and that data are of the type and quality needed to verify protection of the public, employees, and the environment. Figure 9-1 depicts the flow of the QA/QC elements of BNL's Environmental Monitoring Program and indicates the sections of this chapter that discuss each element in more detail.

Laboratory environmental personnel determine sampling requirements using the Environmental Protection Agency (EPA) Data Quality Objective (DQO) process (USEPA 2006), or its equivalent.

Figure 9-1.
Flow of Environmental
Monitoring QA/QC
Program Elements.

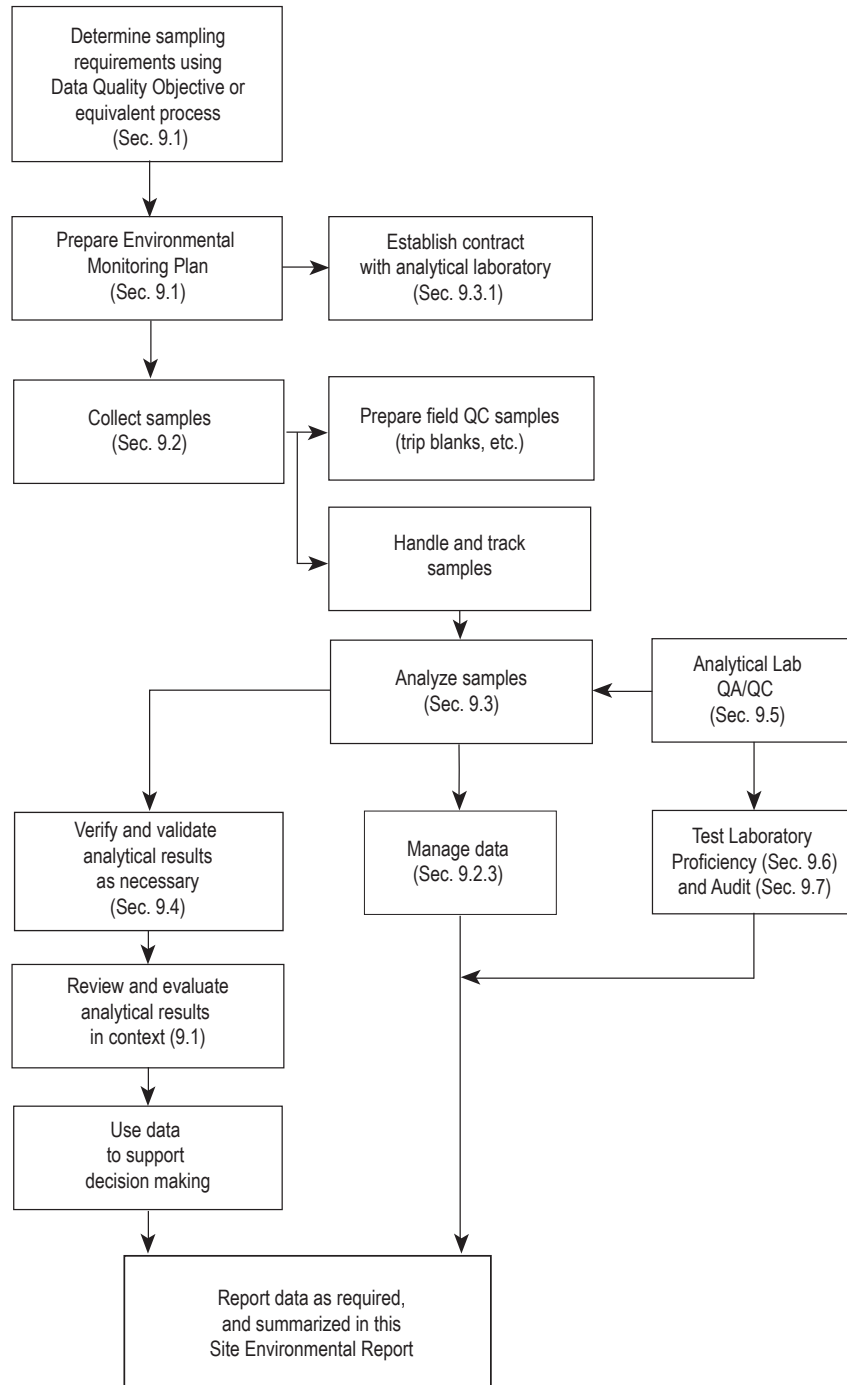

During this process, the project manager for each environmental program determines the type, amount, and quality of data needed to support decision making, legal requirements, and stakeholder expectations. An environmental monitoring plan or project-specific sampling plan is then prepared, specifying the location, frequency, type of sample, analytical methods to be used, and a sampling schedule. These plans and the EM-SOPs also specify data acceptance criteria. Contracts with off-site analytical laboratories are established for sample analysis. The EM-SOPs direct sampling technicians on proper sample collection, preservation, and handling requirements. Field QC samples are prepared as necessary and analyzed in the field or at a certified contract analytical laboratory. The results are then validated or verified in accordance with published procedures.

Finally, the data are reviewed and evaluated by environmental professionals and management in the context of expected results, related monitoring results, historical data, and applicable regulatory requirements (e.g., drinking water standards, permit limits, etc.). The data are used to support decision making, reported as required, and summarized in this annual report.

9.2

Sample Collection and Handling

In 2024, environmental monitoring samples were collected as specified in the Environmental Monitoring Plan Update (BNL 2024a) and project-specific work plans. BNL uses SOPs that are consistent with industry and regulatory standards for the collection of environmental samples, including groundwater, surface water, soil, sediment, air, flora, and fauna. These procedures contain detailed information on the sample collection process, including what types of equipment to use; equipment calibration; how to properly collect, handle, and preserve samples; sample handling and shipment; and how to manage any wastes generated during sampling. QC checks of sampling processes include the collection of field duplicates, matrix spike samples, field blanks, trip blanks, and equipment blanks.

9.2.1 Field Sample Handling

To ensure the integrity of samples, chain of custody (COC) was maintained and documented for all samples collected in 2024. A sample is considered to be in the custody of a person if any of the following rules of custody are met:

1. The person has physical possession of the sample;
2. The sample remains in view of the person after being in possession;
3. The sample is placed in a secure location by the custody holder; or
4. The sample is in a designated secure area.

These procedures are outlined in EM-SOP 109, “Chain-of-Custody, Storage, Packaging, and Shipment of Samples” (BNL 2020).

9.2.1.1 Custody and Documentation

Field sampling technicians are responsible for the care and custody of samples until they are transferred to a receiving group or contract analytical laboratory. Samples requiring refrigeration are placed immediately into a refrigerator or a cooler with cooling media and are kept under custody rules. The technician signs the COC form when relinquishing custody and contract analytical laboratory personnel sign the COC form when accepting custody.

As required by EM-SOP-201, “Documentation of Field Activities” (BNL 2024b), field sampling technicians are also required to maintain bound, weatherproof field logbooks and electronic tablets, which are used to record sample identification (ID) numbers, collection times, descriptions, collection methods, and COC numbers. Daily weather conditions, field measurements, and other appropriate site-specific observations are also recorded in the logbooks.



Groundwater monitoring well sampling in accordance with standard operating procedures.

9.2.1.2 Preservation and Shipment

Before sample collection, field sampling technicians prepare all bottle labels and affix them to the appropriate containers, as defined in the applicable EM-SOPs. Appropriate chemical preservatives are added to the containers before or immediately after collection, and samples are refrigerated as necessary. Sample preservation is maintained, as required, throughout the shipping of the samples to the analytical laboratory.

If samples are sent via a commercial carrier, a bill-of-lading is used. COC seals are placed on the shipping containers and their intact status upon receipt indicates that custody was maintained during shipment.

Upon receipt of the samples, the contract laboratory verifies that proper preservation requirements have been met. BNL is notified as soon as practical if a sample arrives unpreserved, improperly preserved, or at the wrong temperature.

Sample preservations, including incorrect preservation, are noted on the sign-in documentation, and included with every data package. If the BNL Project Manager, with the help of a QC chemist and/or radiochemist, determines that an incorrect preservation issue would result in data that does not meet the data quality objectives of the project, the analysis would be cancelled, and new samples would be collected, as necessary.

9.2.2 Field Quality Control Samples

Field QC samples collected for the environmental monitoring program include equipment blanks, trip blanks, field blanks, field duplicate samples, and matrix spike (MS)/matrix spike duplicate (MSD) samples. The rationale for selecting specific field QC samples, and minimum requirements for their use in the Environmental Monitoring Program, are provided in the BNL EM-SOP 200, "Collection and Frequency of Field Quality Control Samples" (BNL 2022a). Field blanks and trip blanks were collected for all appropriate media in 2024.

An equipment blank is a volume of solution (in this case, laboratory-grade water) that is used to rinse a sampling tool after decontamination. Equipment blank samples are used to verify the effectiveness of the decontamination procedures on non-dedicated or reusable sampling equipment. A trip blank is provided with each shipping container of samples to be analyzed for volatile organic compounds (VOCs). The use of trip blanks provides a way to determine whether contamination of a sample container occurred during shipment from the manufacturer,

while the container was in storage, during shipment to a contract analytical laboratory, or during analysis of a sample at a contract analytical laboratory. Trip blanks consist of an aliquot of laboratory-grade water sealed in a sample bottle, prepared by the contract analytical laboratory or manufacturer prior to shipping the sample bottles to BNL. Trip blanks were included with all shipments of aqueous samples for VOC analysis in 2024.

Field blanks are collected to check for cross-contamination that may occur during sample collection. A field blank consists of an aliquot of laboratory-grade water that is poured into a sample container in the field. For the groundwater monitoring program, one field blank is collected for every 20 samples, or one per sampling round, whichever is more frequent. Field blanks are analyzed for the same parameters as groundwater samples. A Field Reagent Blank (FRB) is collected when analyzing for Per- and Polyfluoroalkyl Substances (PFAS) in groundwater or potable water analyzed using EPA Method 537.1. The FRB must use the same preservative as the samples and is handled the same way as a Field Blank. For other programs, the frequency of field blank collection is based on their specific DQOs.

In 2024, the most common contaminant detected above reporting limit (RL) in the trip, field, and equipment blanks was traced to low levels of styrene, acetone, and methylene chloride (Table 9-1). These commonly observed VOCs are likely due to minor cross contamination of the samples at the analytical laboratory, and their detection does not indicate significant problems with the reliability of the analytical results.

Several other commonly observed compounds were also detected at low levels. When contaminants are detected, validation or verification procedures are used, where applicable, to qualify the associated data as “non-detects” (see Section 9.4). No contamination was detected in the FRBs during 2024. The results from blank samples collected during 2024 did not indicate any significant impact on the quality of the results.

Field duplicate samples are analyzed to check the reproducibility of sampling and analytical results, based on EPA Region II guidelines (USEPA 2024). For example, in the groundwater monitoring program, duplicates are collected for 5% of the total number of samples collected for a project per sampling round.

During 2024, a total of 167 duplicate samples were collected for non-radiological analyses and 101 duplicates were collected for radiologic analyses. Not all parameters were analyzed in every duplicate. The parameters in each duplicate were consistent with those required for the specific program the duplicate was monitoring. Of the 7,981 non-radiologic parameters analyzed, 279 parameters (less than 4%) were above 50% Relative Percent Difference (RPD). For the radiologic parameters, 19 of the 272 parameters (7%) failed to meet criteria. These results are indicative of analytical method consistency within the laboratory, and that consistency within the sample collection process results in valid, reproducible data.

MSs and MSDs are used to determine whether the sample matrix (e.g., water, soil, air, vegetation, or oil) adversely affected the sample analysis. A spike is a known amount of analyte added to a sample. MSs are performed at a rate specified by each environmental program’s DQOs. The rate is typically one per twenty samples collected per project. For 2024, a total of 268 MS/MSD samples were collected for non-radiological analyses and 213 MS/MSD samples were collected for radiological analyses. Not all parameters were analyzed for every MS/MSD pair. Of the 15,447 non-radiological parameters analyzed, 925 parameters (5%) were outside of the QA criteria. For the radiological parameters, 373 of the 503 parameters (74%) meet QA criteria. These overall non-radiological results are indicative of consistent measuring reproducibility with the laboratories and field sampling teams. Radiological results indicate some matrix interference and require more attention to the reported sample results.

Table 9-1. Summary of Detections in Trip, Field, and Equipment Blank Samples.

Constituent	Number of Analyses	Number of Detects	Minimum	Maximum	Typical Reporting Limit	Units
Trip Blank Results						
Methylene chloride	84	8	0.56	2.14	0.5	µg/L
Styrene	84	8	0.18	0.3	0.5	µg/L
Methyl bromide	84	2	0.35	0.37	0.5	µg/L
Naphthalene	84	2	0.38	0.44	0.5	µg/L
1,1,1-Trichloroethane	84	1	0.38	0.38	0.5	µg/L
1,2,3-Trichlorobenzene	84	1	0.37	0.37	0.5	µg/L
Toluene	84	1	0.34	0.34	0.5	µg/L
Field Blank Results						
Organic Compounds						
Methylene chloride	58	8	0.51	1.52	0.5	µg/L
Styrene	58	4	0.3	0.42	0.5	µg/L
Chloroform	58	3	0.26	0.48	0.5	µg/L
cis-1,2-Dichloroethylene	58	1	0.37	0.37	0.5	µg/L
Methyl bromide	58	1	0.28	0.28	0.5	µg/L
Methyl chloride	58	1	0.2	0.2	0.5	µg/L
Metals						
Iron	2	1	32	32	200	µg/L
General Chemistry Parameters						
Ammonia (as N)	2	1	0.05	0.05	0.1	mg/L
Nitrogen	2	1	0.085	0.085	0.1	mg/L
Total Kjeldahl Nitrogen	4	1	0.085	0.085	1	mg/L
Equipment Blank Results						
Organic Compounds						
Perfluorobutyric acid (PFBA)	19	2	0.42	0.71	3.4	ng/L
Perfluorooctanoic acid (PFOA)	19	2	0.61	0.83	1.6	ng/L
Perfluoroheptanoic acid (PFHpA)	19	1	0.84	0.84	1.6	ng/L
Perfluoropentanoic acid (PFPeA)	19	1	1.1	1.1	1.6	ng/L
Acetone	3	3	1.82	3.66	0.5	µg/L
1,4-Dioxane	17	1	0.1	0.1	0.2	µg/L
Metals						
Barium	6	2	3.16	3.97	1	µg/L
Calcium	3	2	89.3	151	50	µg/L
Mercury	30	2	0.28	0.31	0.2	µg/L
Aluminum	3	1	139	139	68	µg/L
Iron	3	1	39.7	39.7	30	µg/L
Lead	6	1	0.0383	0.0383	0.5	µg/L
Potassium	3	1	90.1	90.1	50	µg/L
Zinc	3	1	4.26	4.26	3.3	µg/L

µg/L Micrograms per liter.

mg/L Milligrams per liter.

ng/L Nanograms per liter.



9.2.3 Tracking and Data Management

Most environmental monitoring samples and analytical results were tracked in BNL's Environmental Information Management System (EIMS), a database system used to store, manage, verify, protect, retrieve, and archive BNL's environmental data. Tracking is initiated when a sample is recorded on a COC form. Copies of the COC forms and supplemental forms are provided to the data coordinator to be entered into the EIMS. Each contract analytical laboratory also maintains its own internal sample tracking system (also known as a Laboratory Information Management System).

Following sample analysis, the contract analytical laboratory sends the results to the BNL chemist and project manager for initial review. When required by project-specific DQOs, the analytical data may also be sent to an independent contract chemist for full data validation. Once the results of the analyses are determined to be complete and of acceptable quality, the data are entered into the EIMS. Once entered into EIMS, reports can be generated using a web-based data query tool.

9.3

Sample Analysis

In 2024, environmental samples were analyzed by five contract analytical laboratories, whose selection is discussed in Section 9.3.1. All samples were analyzed according to EPA-approved methods or by standard industry methods where no EPA methods are available (e.g., for tolyltriazole). In addition, during sample collection, field sampling technicians used calibrated field instrumentation for parameters such as conductivity, dissolved oxygen, pH, temperature, and turbidity.

9.3.1 Qualifications

BNL used the following five contract analytical laboratories for analysis of environmental samples in 2024:

1. Chemtex Lab in Port Arthur, Texas, for select non-radiological analytes;
2. General Engineering Lab (GEL) in Charleston, South Carolina, for radiological and non-radiological analytes;
3. PACE Lab in Melville, New York, for non-radiological analytes;
4. Eurofins-Test America (TA), based in Denver, Colorado, for non-radiological analytes; Non-radiological samples were also subcontracted out to TA-Buffalo and TA-Sacramento; Radiological samples from BNL were subcontracted out to TA-St. Louis for radiological analysis; and
5. Eberline Analytical in Oak Ridge, Tennessee, for radiological analytes.

The process of selecting contract analytical laboratories involves the following factors:

- Maintaining required New York State Department of Health (NYSDOH) certifications for the specific analyses to be performed, as applicable;
- Their record on performance evaluation (PE) tests;
- Their contract with the DOE Integrated Contract Procurement Team;
- Pre-selection bidding; and
- Adherence to their own QA/QC programs, which must be documented and provided to BNL.

Routine QC procedures that laboratories must follow, as discussed in Section 9.5, include daily instrument calibrations, efficiency and background checks, and standard tests for precision and accuracy. Four of the five contract laboratories used by BNL in 2024 were certified by the NYSDOH for the relevant analytes, where such certification existed. NYSDOH does not currently certify for the specific analytes tested by Chemtex Lab (e.g., tolyltriazole), which has Texas National Environmental Laboratory Accreditation Program (NELAP) accreditation. The laboratories also were subject to PE testing and DOE-sponsored audits (see Section 9.7).

9.4

Verification and Validation of Analytical Results

Environmental monitoring data are subject to data verification and, in certain cases, data validation when the data quality objectives of the project require this step.

The data verification process involves checking for common errors associated with analytical data. The following criteria can cause data to be rejected during the data verification process:

- **Holding time missed** – The analysis was not initiated, or the sample was not extracted, within the time frame required by EPA or by the contract.
- **Incorrect test method** – The analysis was not performed according to a method required by the contract.
- **Poor recovery** – The chemical compounds or radioisotopes added to the sample before laboratory processing were not recovered at the ratio required by the applicable analytical method/performance criteria.
- **Insufficient QA/QC data** – Supporting data received from the contract analytical laboratory were insufficient to allow for the verification or validation of results.
- **Incorrect minimum detection limit (MDL)** – The contract analytical laboratory reported extremely low levels of analytes as “less than minimum detectable,” but the contractually required limit is not used.
- **Invalid COC** – There was a failure to maintain proper custody of samples as documented on COC forms.
- **Instrument failure** – The analytical instrument did not perform correctly.
- **Preservation requirements not met** – The preservation requirements identified by the specific analytical method were not met or properly documented.
- **Contamination of samples from outside sources** – Possible sources include sampling equipment, personnel, and the contract analytical laboratory.
- **Matrix interference** – Analysis was affected by dissolved inorganic/organic materials in the matrix.

Data validation involves a more extensive process than data verification. Validation includes all the verification checks, as well as checks for common errors, including instrument calibration that was not conducted as required, internal standard errors, transcription errors, and calculation errors. The amount of data that is subjected to the validation process varies, depending on the environmental media and on the DQOs for each project. Data for some projects, such as long-term groundwater monitoring, may require only verification.

The results of the verification and/or validation process are entered into the EIMS. When analyses are determined to be outside of QC parameters, a qualifier is applied to the result stored in the EIMS. Results that have been rejected are qualified with an “R.” Rejected results are not used in the preparation of this report.

The most common QC issue encountered during 2024 was the detection of low-level contamination in the trip, field, and method blanks used in VOC analyses. Results for the trip, equipment, and field blanks are summarized in Table 9-1. This issue resulted in minor qualifications of sample results. Also, minor violations of laboratory control sample results were also common. In most cases, the violations do not result in qualified sample results.

9.4.1 Checking Results

Non-radiological data analyzed in 2024 were verified and/or validated when required by project DQOs, BNL EM-SOPs, and/or EPA contract laboratory program guidelines (USEPA 2000). Radiological packages were verified and/or validated using BNL and DOE guidance documents (BNL 2022b). During 2024, the verifications were conducted using a combination of manually checking data packages and by the use of a computer program developed by BNL to verify the completeness of electronic data deliverables (EDDs) before the data are entered into BNL's EIMS.

9.5

Contract Analytical Laboratory QA/QC

In 2024, procedures for calibrating instruments, analyzing samples, and assessing QC were consistent with EPA methodology. QC checks performed included: analyzing blanks and instrument background; using Amersham Radiopharmaceutical Company or National Institute for Standards and Technology (NIST) traceable standards; and analyzing reference standards, spiked samples, and duplicate samples. Analytical laboratory contracts specify analytes, methods, required detection limits, and deliverables, which include standard batch QA/QC performance checks.

As part of the laboratory selection process, candidate laboratories are required to provide BNL with copies of their QA/QC manuals and QA program plans. Nonconformance reports are generated when discrepancies are found in field sampling designs, documented procedures, COC forms, data analyses, data processing systems, and QA software, or when failures in Proficiency Evaluation (PE) testing occur. Following investigation into the root causes, corrective actions are taken and tracked to closure.

9.6

Performance or Proficiency Evaluations

All the contract analytical laboratories (Chemtex, Eberline, GEL, PACE, and TA) participated in several national and state PE testing programs in 2024. Chemtex Lab participated in PE testing for total phosphorus, which is used to determine one of the specific analytes Chemtex analyzed for BNL (specifically for tolyltriazole, polypropylene glycol monobutyl ether, and 1,1-hydroxyethylidene diphosphonic acid). Each of the participating laboratories took part in at least one testing program, and several laboratories participated in multiple programs. Results of the tests provide information on the quality of a laboratory's analytical capabilities.

The testing was conducted by Environmental Resource Associates (ERA), the DOE Mixed Analyte Performance Evaluation Program (MAPEP), Resource Technology Corporation, Phenova, and the NYSDOH Environmental Laboratory Accreditation Program (ELAP). The results from these tests are summarized in Section 9.6.

9.6.1 Summary of Test Results

As shown by Figures 9-2 and 9-3, test results are plotted as percentage scores that were “Acceptable,” “Warning (But Acceptable),” or “Not Acceptable.” A Warning (But Acceptable) is considered by the testing organization to be “satisfactory.” An “Average Overall Satisfactory” score is the sum of results rated as Acceptable and those rated as Warning (But Acceptable), divided by the total number of results reported. A Not Acceptable rating reflects a result that is greater than three standard deviations from the known value—a criterion set by the independent testing organizations.

Table 9-2 provides a summary of the DOE’s Consolidated Audit Program (DOECAP) audit results. The TA-St. Louis lab had one Priority II finding; Eberline had 1 Priority II finding; GEL had 1 Priority I finding. Chemtex, GEL, and PACE were not audited for 2024 for DOECAP. Priority II findings are deviations from a requirement. Priority I findings are issues that present substantial risk if not resolved in an expedited manner. Resolution/impacts of these findings are discussed in Section 9.7.

Table 9-2. Summary Results of 2024 DOECAP Audits.

Laboratory	Finding Priority	Area of Concentration	Number of Findings
Eurofins/Test America, St. Louis, Missouri December 6-8, 2023	II	Radiochemistry	2
	NA	Quality Assurance	NA
	NA	Organic Analyses	NA
	NA	Inorganic Analyses and Wet Chemistry	NA
	NA	Laboratory Information Management Systems	NA
	NA	Materials Management	NA
GEL Laboratories, Charleston, South Carolina February 20-21, 2024	NA	Radiochemistry	NA
	NA	Quality Assurance	NA
	I	Organic Analyses	1
	NA	Inorganic Analyses and Wet Chemistry	NA
	NA	Laboratory Information Management Systems	NA
	NA	Materials Management	NA
Eberline Analytical Corp., Oak Ridge, Tennessee May 29-31, 2024	NA	Radiochemistry	NA
	II	Quality Assurance	1
	NA	Organic Analyses	NA
	NA	Inorganic Analyses and Wet Chemistry	NA
	NA	Laboratory Information Management Systems	NA
	NA	Materials Management	NA


NA Not applicable.

9.6.1.1 Radiological Assessments

Figure 9-2 summarizes radiological performance scores in the ERA and MAPEP programs for 2024. Eberline, GEL and TA participated in the ERA radiological PE studies with Eberline having an average overall score of 76%. GEL had an average overall score of 96%. TA also had an overall score of 93%. GEL scored 92% in the MAPEP program, while Eberline had 82%. TA no longer participates in the MAPEP tests. Chemtex and PACE did not analyze radiological samples for BNL.

Figure 9-2.

Summary of Scores in the Radiological Proficiency Evaluation Programs.

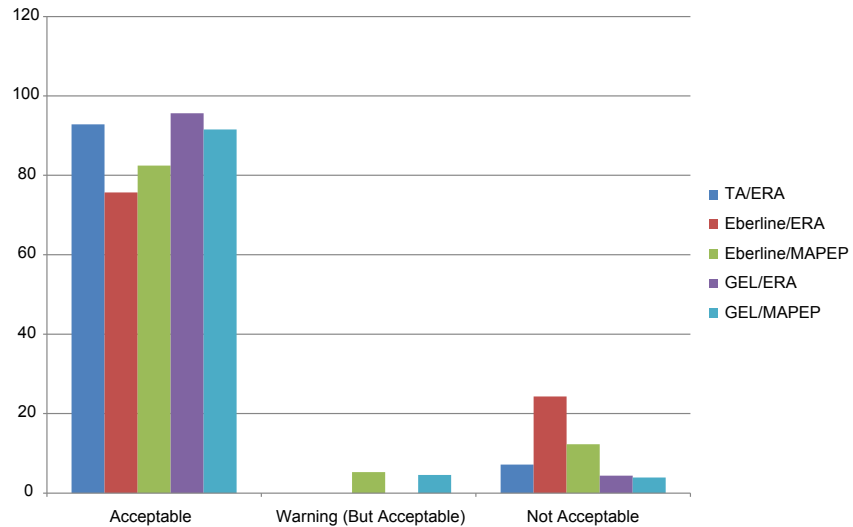


9.6.1.2 Non-radiological Assessments

Figure 9-3 summarizes the non-radiological performance results of three participating laboratories (GEL, Pace, and TA) in the ERA, MAPEP, Phenova, and ELAP tests. During 2024, PACE participated in the NYSDOH ELAP evaluations of performance on tests of non-potable water, potable water, and solid wastes. NYSDOH found 98% of PACE's non-radiological tests to be in the Acceptable range. GEL participated in the ERA program for non-potable water, potable water, and solid wastes and received a score of 99%. GEL also scored 90% in the MAPEP TA participated in the ERA and Phenova programs for non-potable water, potable water, and solid wastes with scores of 99% and 99%, respectively.

Figure 9-3.

Summary of Scores in the Non-radiological Proficiency Evaluation Programs.

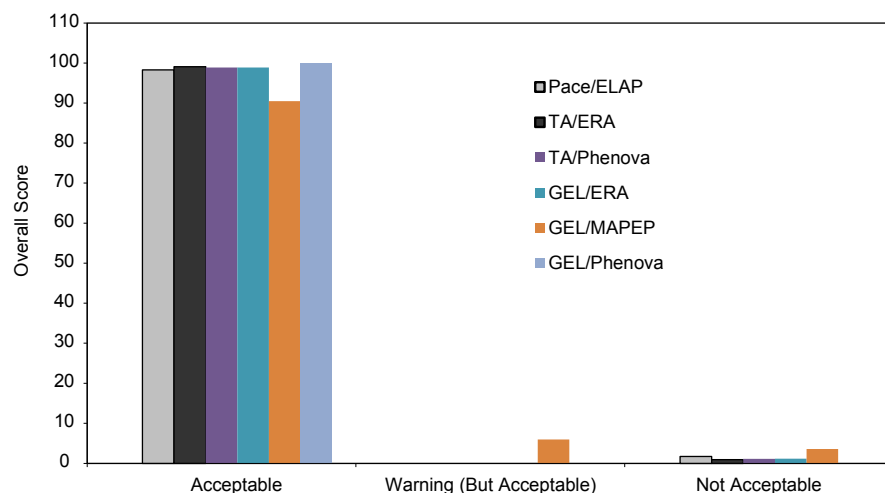

9.7

Audits

As part of DOECAP, TA-St. Louis was audited in December 2023 (ANAB 2023) by American National Standards Institute-American Society for Quality (ANSI-ASQ) National Accreditation Board (ANAB). During the audits, one nonconformity was cited in radiochemistry. This finding did not affect the quality of BNL's data.

GEL was re-audited in February 2024 (ANAB 2024a) by ANSI-ASQ ANAB. This was a follow up of the 2023 DOECAP audit. One nonconformity in Organics was found. This finding did not affect the quality of BNL's data.

Eberline was audited in May 2024 (ANAB 2024b) by ANSI-ASQ ANAB. During the audits, one nonconformity was cited in Quality Control. This finding did not affect the quality of BNL's data.

Chemtex and PACE were not assessed for DOECAP during the 2024 calendar year. Based on the audit, assessments, and corrective action response, the analytical laboratories met the criteria of the audit programs for Acceptable status.

9.8

Conclusion

The data validations and data verifications conducted on analytical results are designed to eliminate data that fails to meet the DQOs of each project. The results of the independent PE assessments and assessments of contractor laboratories summarized in this report are also used to assess the quality of the results. As a result of these assessments, BNL has determined that the data used in this SER are of acceptable quality.

References and Bibliography

- USEPA. 2006a. Guidance on Systematic Planning Using the Data Quality Objectives Process. EPA QA/G-4, EPA/240/B-06/001, U.S. Environmental Protection Agency, Office of Environmental Information, Washington DC
- USEPA 2024, Region 2 Quality Assurance Guidance and Standard Operating Procedures, Retrieved September 6, 2024, from <https://www.epa.gov>.
- 10CFR 830 Subpart A. U.S. Department of Energy. Quality Assurance Requirements. U.S. Code of Federal Regulations. 2000.
- ANAB 2023. 2023 DOECAP Accreditation Program Assessment Report for Eurofins Test America Laboratories, Inc.-St. Louis, Missouri, December 2023
- ANAB 2024a. 2024 DOECAP Accreditation Program Assessment Report for GEL Laboratories, LLC.-Charleston, South Carolina, February 2024
- ANAB 2024b. 2024 DOECAP Accreditation Program Assessment Report for Eberline Analytical Corporation.-Oak Ridge, Tennessee, May 2024
- BNL 2020. EM-SOP 109. Chain-of-Custody, Storage, Packaging, and Shipment of Samples. Brookhaven National Laboratory. Upton, NY.
- BNL 2022a. EM-SOP 200. Collection and Frequency of Field Quality Control Samples. Brookhaven National Laboratory, Upton, NY
- BNL 2022b. EM-SOP 209. Radiochemical Data Validation. Brookhaven National Laboratory, Upton, NY.
- BNL 2024a. Brookhaven National Laboratory Environmental Monitoring Plan Update. Brookhaven National Laboratory, Upton, NY. January 2024.
- BNL 2024b. EM-SOP-201 Documentation of Field Activities. Brookhaven National Laboratory, Upton, NY.
- DOE Order 414.1D. Quality Assurance. U.S. Department of Energy. Washington, DC. August 16, 2011.
- DOE Order 458.1. Radiation Protection of the Public and Environment. U.S. Department of Energy. Washington, DC. February 11, 2011.

