

***Cryogenic System for BEPCII SRF Cavity, IR  
Quadrupole and Detector Solenoid Magnets***

**L. X. Jia et al**

*Presented at the 20<sup>th</sup> International Cryogenic Engineering  
Conference & Exhibition  
Beijing, China  
May 11-14, 2004*

July 2004

**Collider-Accelerator Department**

**Brookhaven National Laboratory**

P.O. Box 5000  
Upton, NY 11973-5000  
[www.bnl.gov](http://www.bnl.gov)

*Managed by*  
Brookhaven Science Associates, LLC  
for the United States Department of Energy under  
Contract No. DE-AC02-98CH10886

## DISCLAIMER

This report was prepared as an account of work sponsored by an agency of the United States Government. Neither the United States Government nor any agency thereof, nor any of their employees, nor any of their contractors, subcontractors, or their employees, makes any warranty, express or implied, or assumes any legal liability or responsibility for the accuracy, completeness, or any third party's use or the results of such use of any information, apparatus, product, or process disclosed, or represents that its use would not infringe privately owned rights. Reference herein to any specific commercial product, process, or service by trade name, trademark, manufacturer, or otherwise, does not necessarily constitute or imply its endorsement, recommendation, or favoring by the United States Government or any agency thereof or its contractors or subcontractors. The views and opinions of authors expressed herein do not necessarily state or reflect those of the United States Government or any agency thereof.

### FOR UNCLASSIFIED, UNLIMITED STI PRODUCTS

Available electronically at:

#### OSTI:

<http://www.osti.gov/bridge>

Available for a processing fee to U.S. Department of Energy and its contractors, in paper from:

U.S. Department of Energy  
Office of Scientific and Technical Information  
P.O. Box 62  
Oak Ridge, TN 37831  
Phone: (865) 576-8401  
Facsimile: (865) 576-5728  
E-mail: [reports@adonis.osti.gov](mailto:reports@adonis.osti.gov)

#### National Technical Information Service (NTIS):

Available for sale to the public from:

U.S. Department of Commerce  
National Technical Information Service  
5285 Port Royal Road  
Springfield, VA 22131  
Phone: (800) 553-6847  
Facsimile: (703) 605-6900  
Online ordering: <http://www.ntis.gov/ordering.htm>

## **Cryogenic System for BEPCII SRF Cavity, IR Quadrupole, and Detector Solenoid Magnets\***

Jia L.X.<sup>1</sup> and Wang L.<sup>2</sup>

<sup>1</sup>Brookhaven National Laboratory, Upton, New York 11973, USA

<sup>2</sup>Institute of Cryogenics and Superconductivity Technology, Harbin Institute of Technology, Harbin 150001, CHINA

Beijing Electron-Positron Collider Upgrade (BEPCII) requires three types of superconducting facilities, including one pair of SRF cavities, one pair of interaction region quadrupole magnets, and one detector solenoid magnet. The cryo-plant for BEPCII has a total cooling capacity of 1kW at 4.5K, which is composed of two separate helium refrigerators of 500W each. Two refrigerators share the same gas storage and recovery system. The engineering design for the cryogenic systems, including power leads, control dewars, subcooler, cryogenic valve boxes, cryogenic transfer-lines and cryogenic controls, is completed. The production of its subsystem is under way. This paper summarizes the progress in cryogenics of the BEPCII project.

### **INTRODUCTION**

The cryogenic facilities in the BEPCII cryoplant are distributed in four areas; the first colliding hall, the second colliding hall, the compressor hall, and the gas tank farm (see Figure 1). The BESIII detector solenoid magnet and a pair of interaction region quadrupole magnets are located in the first colliding hall. The two SRF cavities are located in the second colliding hall. The two colliding halls are in a distance of 100 meters. To reduce the length of cryogenic transfer line and to meet the different loading requirements in two operation modes, colliding mode and the synchrotron radiation mode, the two separate helium refrigerators of 500W each are used for each colliding hall [1,2].

### **THE FIRST COLLIDING HALL**

The layout of the cryogenic subsystem in the first colliding hall is shown in Figure 2. There are three superconducting facilities: the detector solenoid magnet with its valve box and two quadrupole magnets with separated valve box. To support these facilities, a 500W helium refrigerator (Linde TCF50) and a 1000 liter liquid helium control dewar are installed in the adjacent refrigerator building. The liquid helium produced by the refrigerator cold box is delivered to the subcooler that serves the control dewar. On the top of the subcooler is a cryogenic valve box that serves as a distributor to deliver subcooled helium to the valve boxes of the detector magnet and the two quadrupole magnets. The valve box for each magnet contains the power leads, cryogenic valves, relief valves, and pressure and temperature instrument ports. The vacuum jacketed cryogenic transfer lines among these valve boxes are the type of multiple lines for helium and nitrogen. The multiple transfer line between quadrupole magnet and its valve box also contains the superconducting cables. The quench gas return lines and lead cooling gas return lines run bypassing the refrigerator to the compressor suction. The high pressure warm gas lines and low

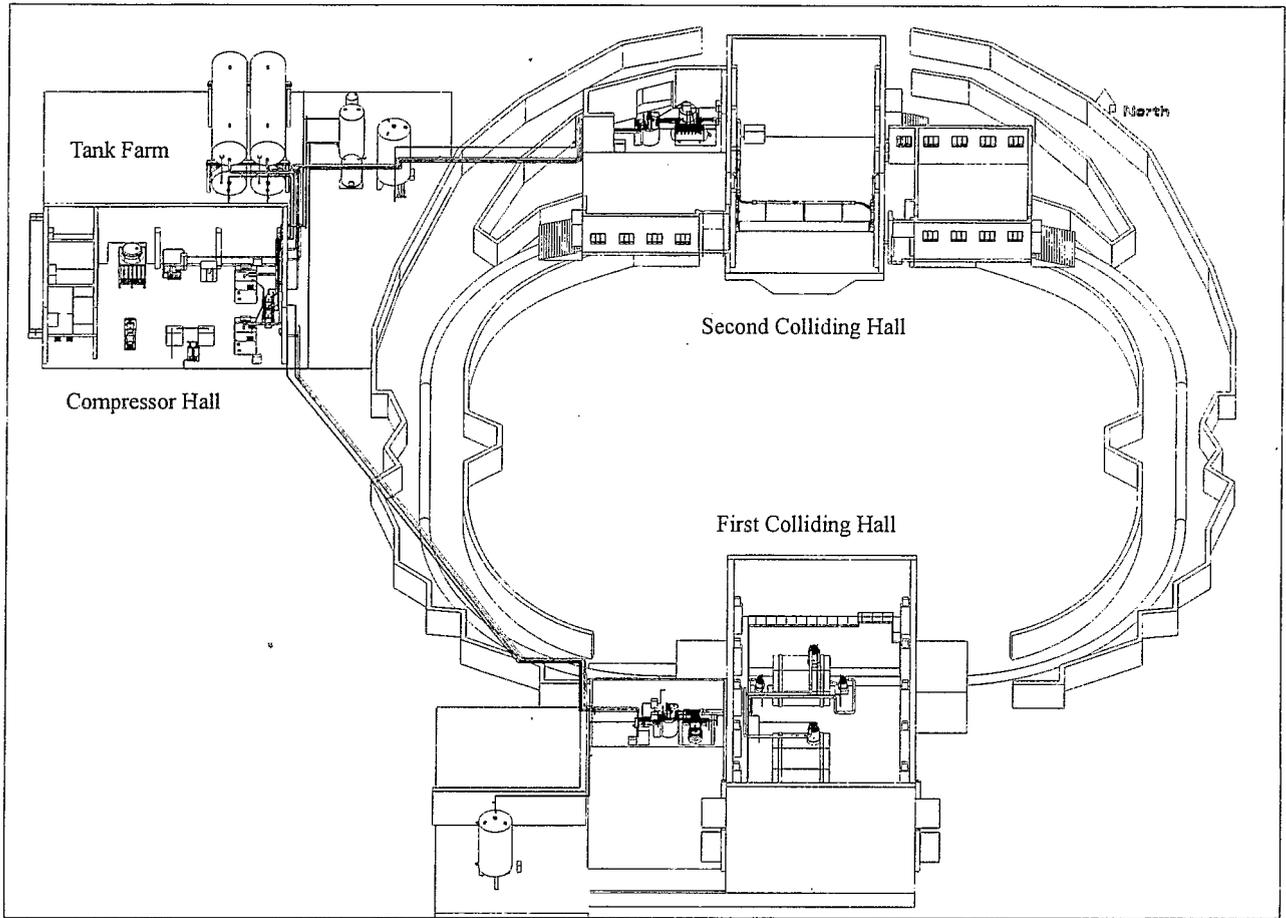


Figure 1 BEPCII ring and its cryogenic facilities

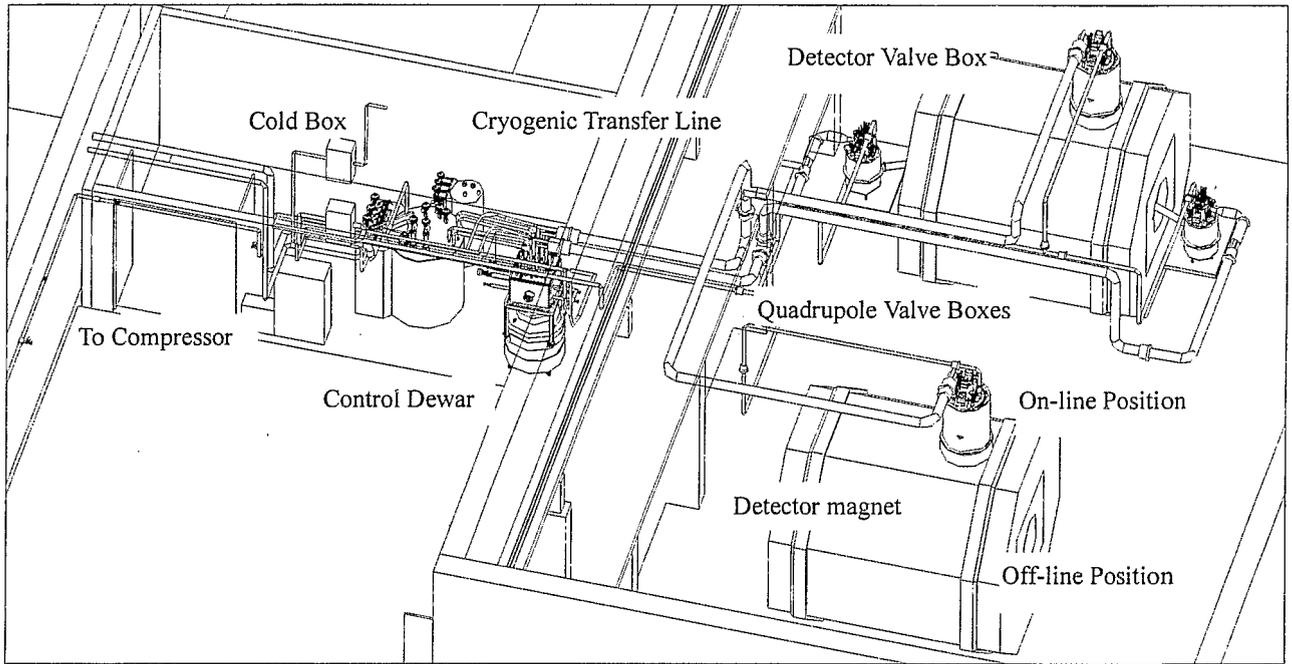


Figure 2 The first colliding hall and its cryogenic system

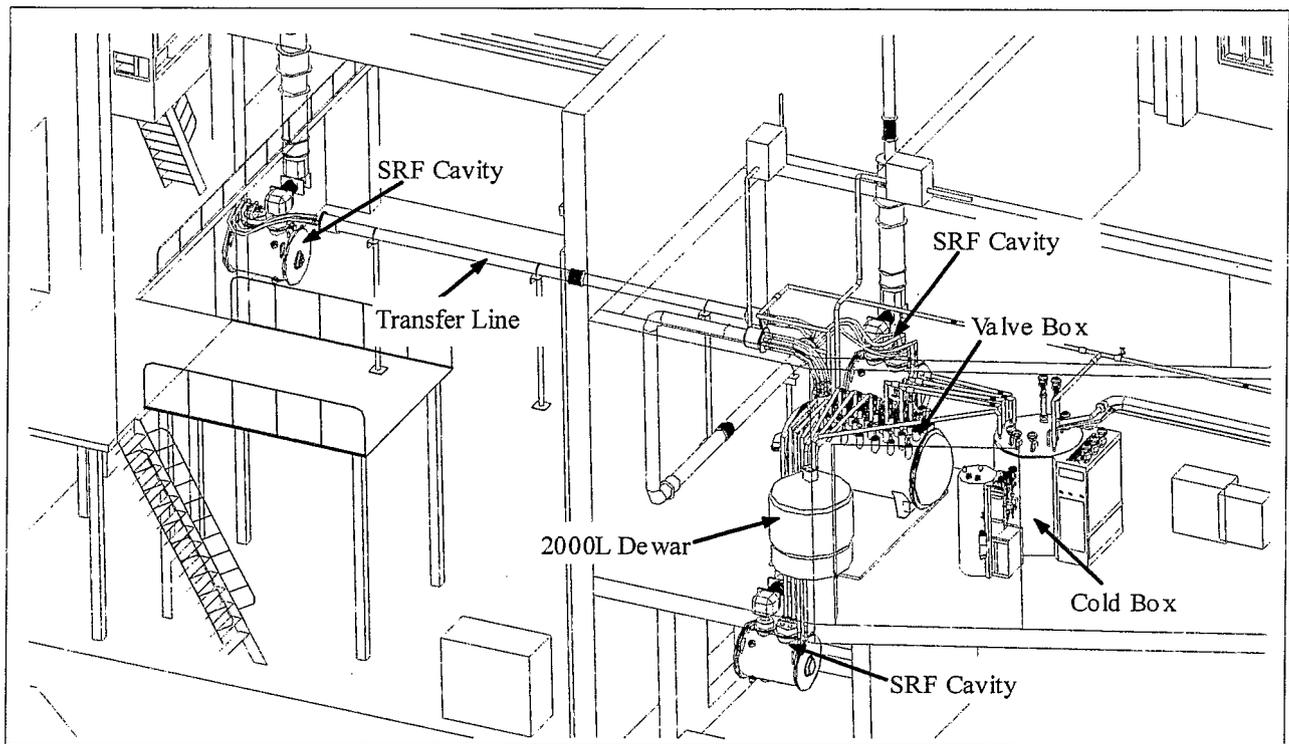


Figure 3 The second colliding hall and its cryogenic system

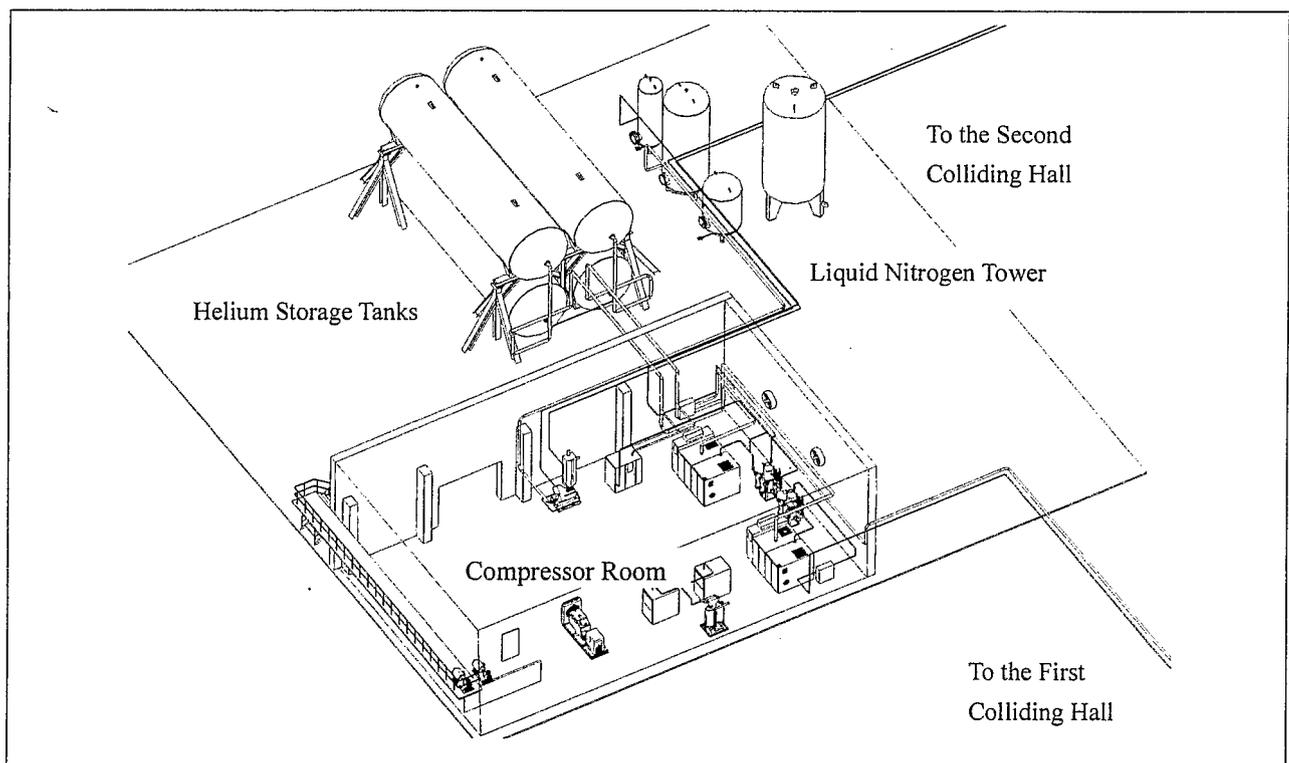


Figure 4 Compressor room and gas tank farm

pressure warm gas line run from the cold box to remotely located compressor building. A liquid nitrogen tower for the refrigerator cold box and magnet heat shield is located just outside of the first colliding hall. The vacuum jacketed transfer lines for the detector solenoid magnet is designed to accommodate its off-line test positions as well as the in-line operation position. The vacuum separation barriers are arranged in various portions of the transfer lines that allows the quick reassemble and relocation of each cry modules.

## THE SECOND COLLIDING HALL

The layout of the cryogenic subsystem in the second colliding hall is shown in Figure 3. Three superconducting RF cavities: two in-lined cavities and one off-line test cavity. In the refrigerator building adjacent to the second colliding hall, there are four major cryo equipments: the refrigerator cold box with the cooling capacity of 500W (Linde TCF50), the external cryogenic helium purifier, the 2000 liter liquid helium dewar, and the SRF distribution valve box. The 2000 liter dewar is used to maintain available liquid helium for each cavity for cool down and operation. Each cavity has a liquid volume of 300 liters. The main cryogenic valve box distributes liquid to three SRF cavities. The valve box is so designed that three cavities can be cold at the same time or anyone of three cavities can be cold when others are warm. This horizontal valve box contains all necessary cryogenic valves, relief valves, and pressure sensor ports. The multiple cryogenic transfer lines in the second colliding hall are designed with several vacuum barriers for operating and testing of these cavities.

## THE COMPRESSOR HALL AND TANK FARM

The layout of the helium compressor hall and the helium gas tank farm is shown in Figure 4. The compressor hall is remotely located in a new building that is about 100 meters away from the first colliding hall and 70 meters away from the second colliding hall. Two compressors with separated oil removal, cooling water, and VFD systems are located in the compressor hall. Each compressor supports each cold box in the first and the second colliding halls. The piping for the two compressors is designed as to support individual cold box at different colliding hall and also to be the backup of each other. The compressor hall also contains the instrument air pumping system and the emergency electrical power generator. The cryogenic control room for the entire cryoplant is also located in the same building. Adjacent to the compressor hall is the tank farm in which there are four high pressure gas tanks, 130 m<sup>3</sup> each, one impurity helium gas tank, one instrument air tank, and one liquid nitrogen tower of 30 m<sup>3</sup> in capacity.

## CONCLUSION

The engineering design work for the BEPCII cryogenic system is carried out in the framework of collaboration among three institutes: the Institute of High Energy Physics, the Institute of Cryogenics and Superconductivity Technology, and the Brookhaven National Laboratory. The design work started in March 2003 and basically completed in May 2004. The construction will be soon started as this report is presented. The mechanical fabrication of the cryogenic system is to be conducted in China with some imported components such as the refrigerators and cryogenic valves.

## REFERENCES

1. Jia, L.X. and Wang, L., 1kW Cryoplant for BEPCII Superconducting Facilities, Proceedings of ICCR'2003, Hangzhou, China (2003) 47-50
2. Jia, L.X. and Wang, L., Cryogenics in BEPCII Upgrade, Proceedings of ICEC-19 Grenoble France (2002) 39-42